

美迪西微信

浦东新区川大路585号 | 3
marketing@medicilon.com.cn

00-780-8018 (中国大陆) | +86 (21)

2004 CRO()
2019 11 5 CRO
688202

10
AAALAC
80%
NMPA GLP
30%
FDA GLP
U•



2004 -2008

-
-
- 2

2008
GLP

2009 -2014



- ()
-
- GLP
- AAALAC
-

NMPA US FDA IND CRO


2015 -

- FDA GLP
-
-

2019 11 5
ADC

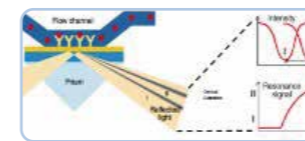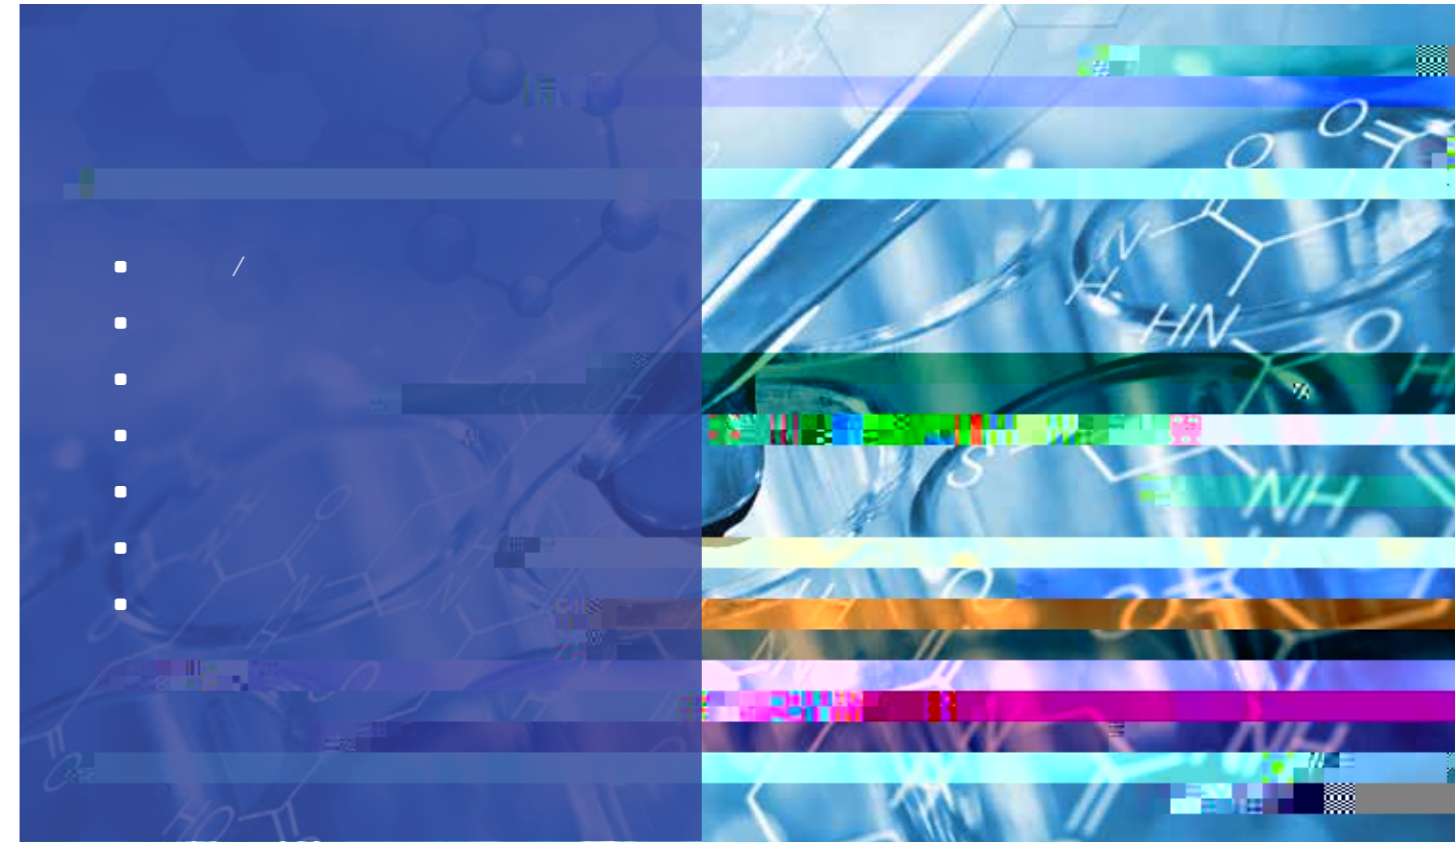


Biacore



PROTAC

RNAi CAR-T

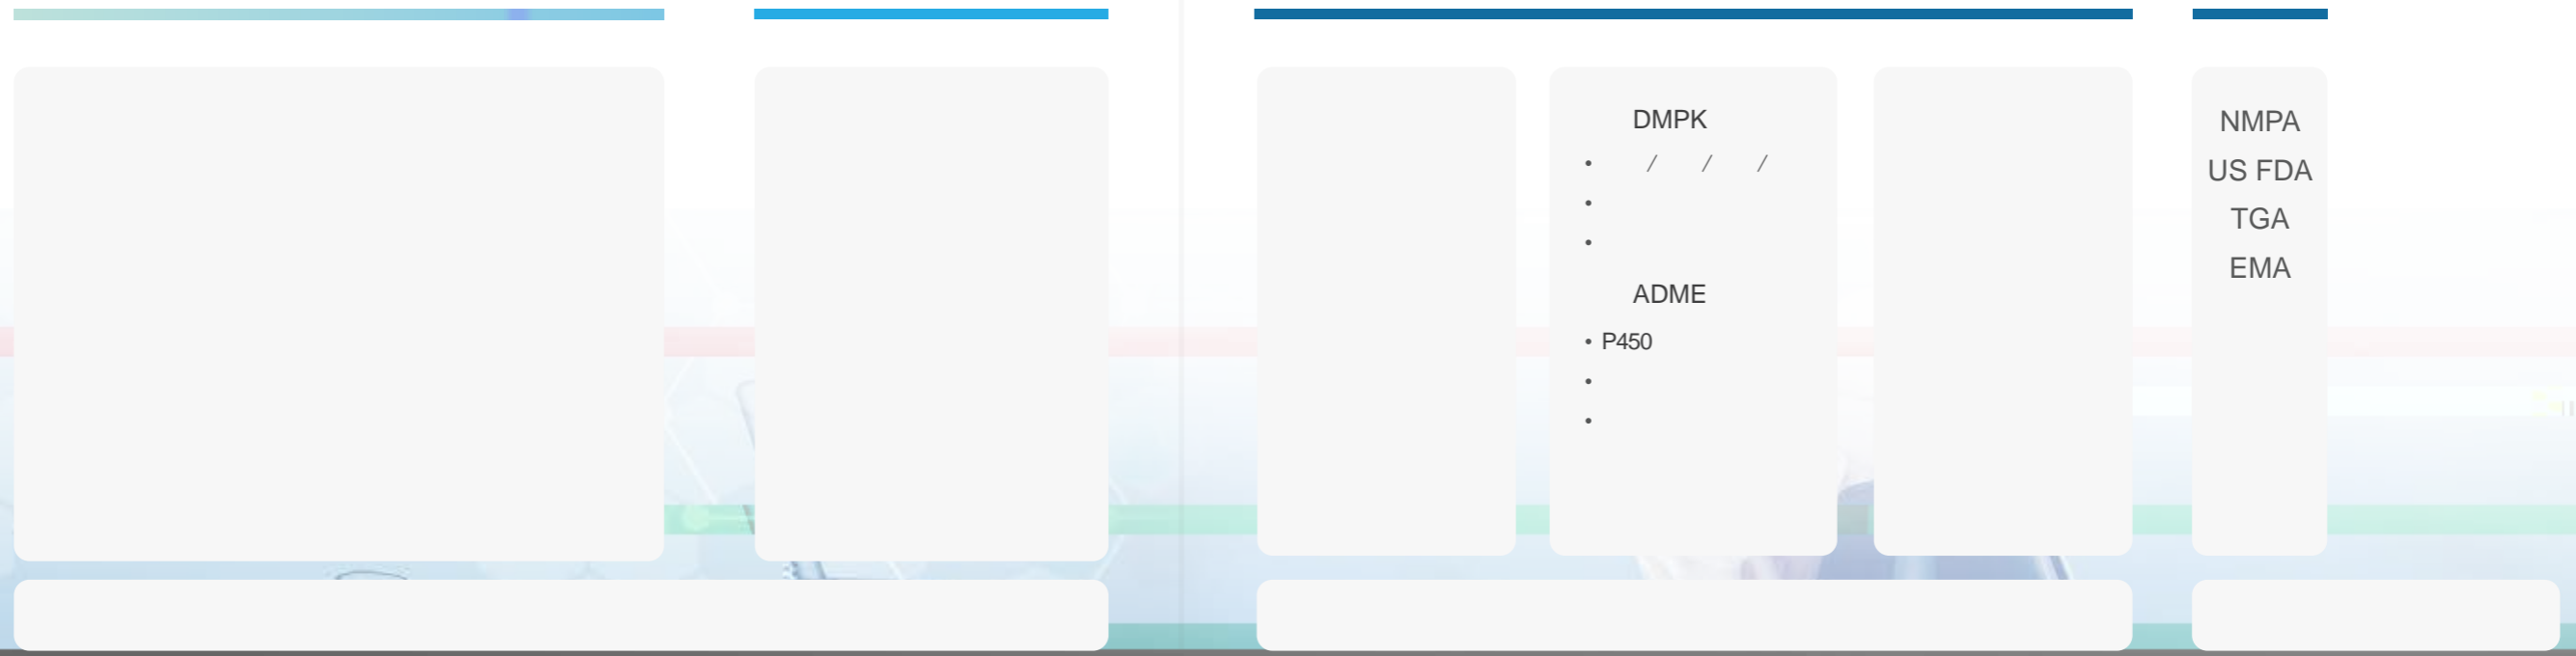



GMP

CRO

CDMO

API

API

API

DMF

(QbD)

API



01

5-10

02

BE

API
100%

API

03


2 cGMP
BE

IND


04

API


KNOW

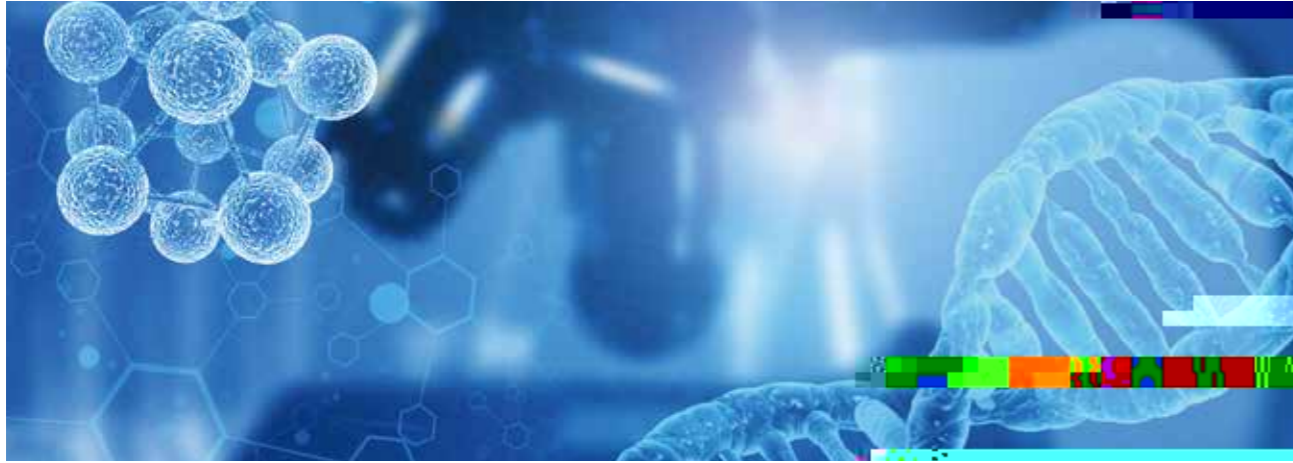




- 01
- 02
- 03
- 04
- 05




~186 ~30 ~30 ~50 ~100	PDX Models	~64 ~32 ~25 ~18 ~39
-----------------------------------	------------	---------------------------------




<ul style="list-style-type: none">/	<ul style="list-style-type: none">(含hERG测试)	<ul style="list-style-type: none">HEIHC)TCR)	<ul style="list-style-type: none">
--	---	--	--

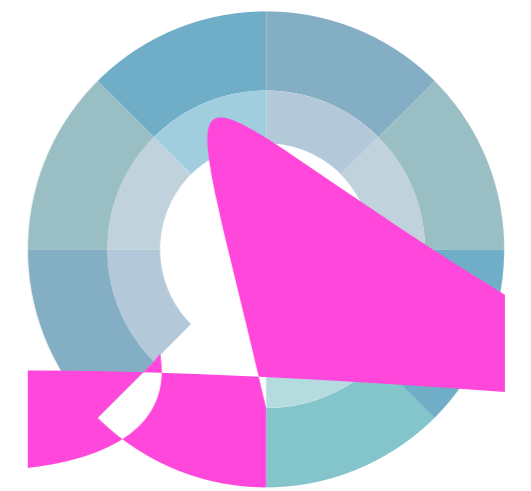




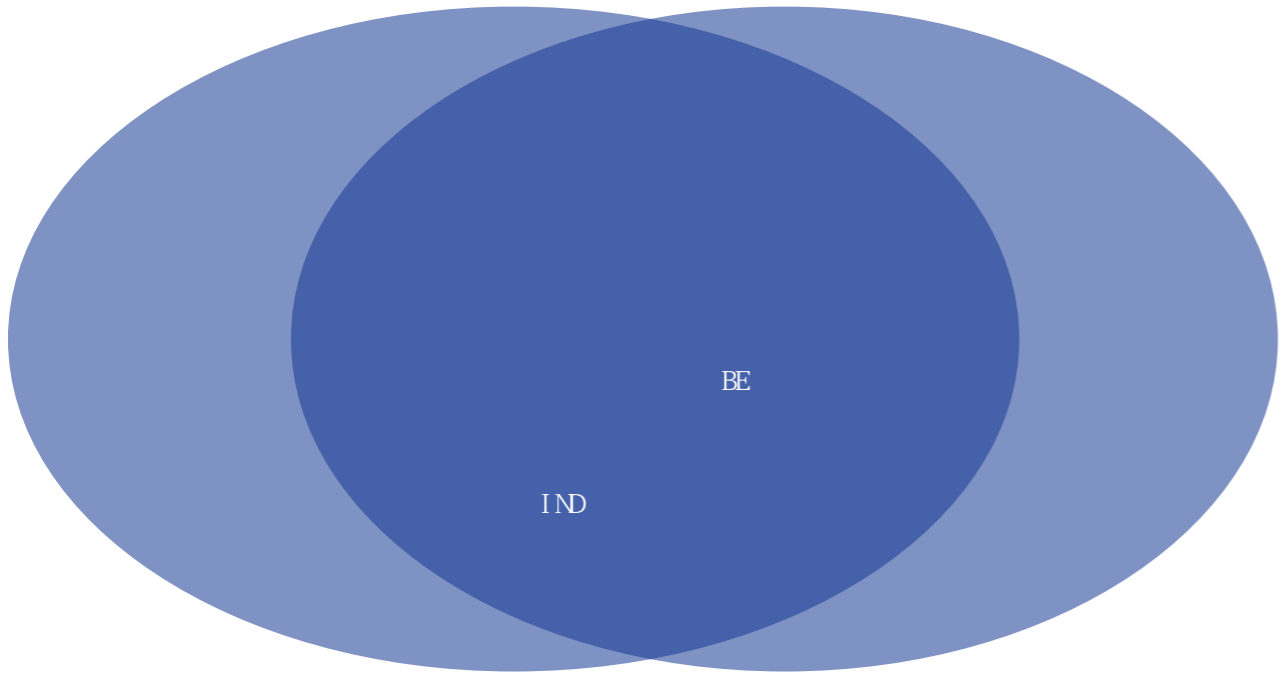

IND

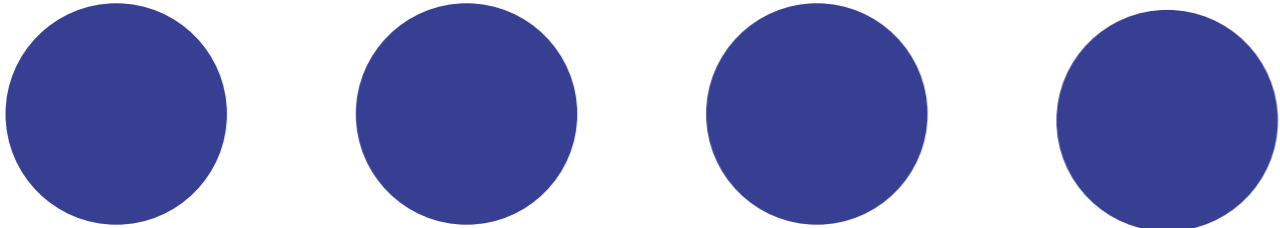

	:
38 FTEs ()
2-3	HTS
5	1

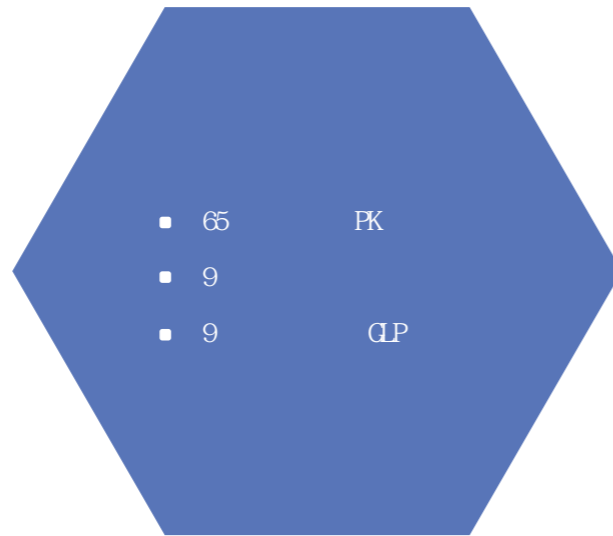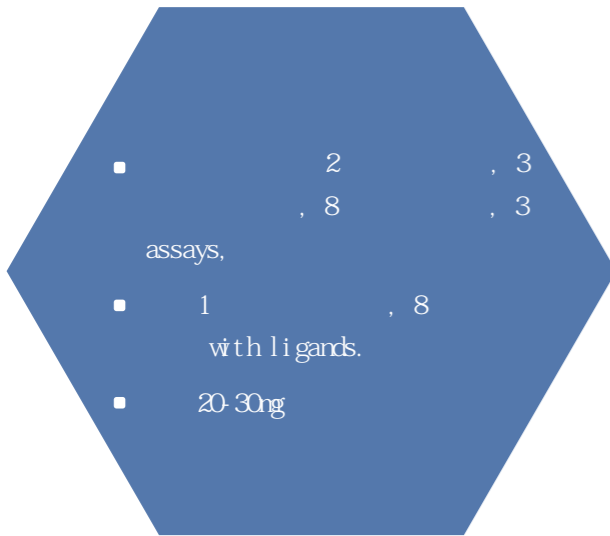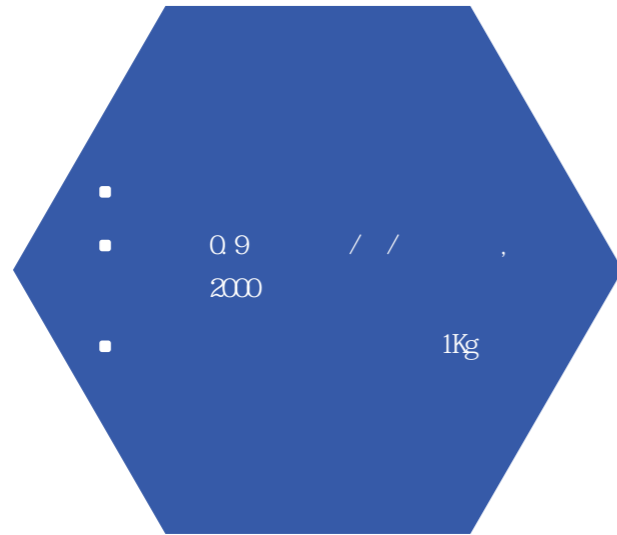

Dark blue header bar

Large empty light gray box

Dark blue header bar

4 4

Dark blue header bar

5
PK/PD

Dark blue header bar

SD
SD
CYP

Caco-2

Dark blue header bar

MMPA
FDA

SEND